



EMS MEMORIAL CO-OPERATIVE HOSPITAL & RESEARCH CENTRE, PERINTHALMANNA

NABH Accredited and ISO 9001-2015 Certified Multi Super Speciality Hospital

P.B. No. 25, PERINTHALMANNA - 679 322.

PHONE: 04933 225751-225755, 276 000, 353 000

email : info@emshospital.org.in, emshospital@rediffmail.com website : www.emshospital.org.in



EMCH / QTN / GEN / 4/ 2026

4th June 2026

QUOTATION NOTICE FOR PURCHASE OF BED SIDE LOCKER & CRASH CART TROLLEY

Sealed quotations are invited from reputed manufacturers / authorised suppliers / dealers for the supply of plastic items as per the list attached :

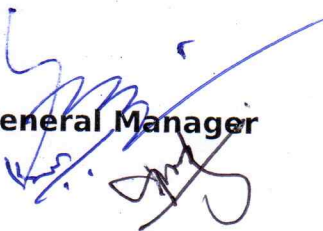
1	<p><u>Bedside Locker</u></p> <ol style="list-style-type: none">1. Overall Size: 1015 mm L x 510 mm W x 920 mm H. (± 10 mm Variation)2. Shelf Size: 755 mm L x 500 mm W. (± 10 mm Variation)3. Verticals made of 31.75 mm OD x 1.2 mm (18 G) S S tube. Horizontal stays made of 19.05 mm OD x 1.2 mm (18 G) S S tube with S S tube 15.87 mm x 1.2 mm (18 G) on all four sides to support two stainless steel shelves0.9 mm (20 G) over with 10 mm dia rod stainless steel railings shall be provided on all four sides. The height of railing is 3" (75 mm).4. Verticals mounted on 125 mm dia non -rusting castor two with brakes and two without brakes.5. Castor made from high grade non-floor-staining synthetic materials with integrated thread guards. Wheel centre having precision ball bearing to run smoothly.6. Two stainless steel shelves of 0.9 mm (20 G) thickness, with protective railings on four sides. The railing shall be made from dia 10mm S.S. Rod.7. The distance between the two shelves is 460 mm and distance from ground to bottom shelf is 330 mm.8. The trolley shall hold seamless stainless-steel bucket with S.S. lid at lower level and S.S. bowl at top level respectively.9. The size of bucket is 230 mm H x 250 mm Outer diameter and size of bowl is 250 mm OD x 85 mm H. Both are made from SS 304 sheet 0.5 mm (25 G)10. Both removable bowl and bucket are mounted on the removable SS frame made from 10 mm diameter rod. This SS frame is assembled on SS sleeve which is	125 Nos
---	--	---------

	<p>welded to vertical tube.</p> <p>11. Only 304 grade stainless steel should be used for tubular frame work & SS shelves of trolley. The trolley shall be in matt finish.</p> <p>12. SS parts finished with Matt Polish.</p> <p>13. Load bearing capacity: 50 kgs (Per Shelf - 25 Kgs).</p> <p>14. Should have ISO 9001 certification</p>	
2	<p>SS Crash Cart Trolley</p> <p>A) Technical Specifications:</p> <p>It should fulfil all the requirements as per Technical Specifications given below:</p> <ol style="list-style-type: none"> 1. Size should be 960 mm L x 500 mm W X 1545 MM H. 2. The crash cart should have Stainless steel tubular frame work. 3. 6 Nos. hand out Bins to keep important supplies easily accessible. 4. Total Three S.S. shelves with railing to carry medicine equipment's 5. Facility to carry monitors, ECG, suction apparatus on open areas at top center and bottom shelves. 6. One wooden writing board. 7. Stainless steel saline rod made of 12 mm dia. 304 grade S.S. approx. 750 mm long and bent at top to have an arm of 400 mm approx. at the end of which of 6 mm dia. S.S. hook shall be welded with TIG process. 8. Crash cart with 125 or 150mm dia. non-rusting imported castor wheels two with brakes and two without. Castor housing and wheels made from high grade non floor staining synthetic materials with integrated thread guards. Wheel center having precision ball bearing to run smoothly, provided with round buffer, one on each corner. 9. Massage board for cardiac patient are provided. It shall have water resistance property and it should be made from ecofriendly material. 10. Oxygen cylinder stand epoxy powder coated one side. All MS parts are passed through 8 tanks Pretreated & powder coated process. SS parts finished with Matt polish 11. Warranty: Should have 3yrs. of manufacturer warranty 12. Manufacturer should be ISO 9001 certified. 13. Product should have European CE certified by a notified body/BIS/ USFDA/ 	20 Nos

	<p>CDSCO license/ISO 13485:2016 from any notified body (such as NABCB/CDSCO/CE).</p> <p>14. It Should furnish stainless steel grade certificate from Govt/Govt approved laboratory for test procedure.</p> <p>15. The manufacturer should have ISO 13485:2016 certifications.</p>	
--	---	--

1. Quotations should be in Two sealed covers
First cover superscribed " Technical cover" should include technical specifications, list of supplied-institutions with contact numbers of end users, authorization for the supply, certifications such as License, Dealership etc.
2. Second cover super scribed "Commercial cover" should include commercial terms such as Price, Warranty terms, tax if any, etc.
3. Technical details will be scrutinized by a technical committee. Technically qualified quotations will only be considered for opening of Commercial cover.
4. The quotationers if they are suppliers they should submit their authorization for supply of the quoted items from the Manufacturer

Sealed quotations addressed to The General Manager, EMS Memorial Cooperative Hospital, Perinthalmanna should reach the Administrative Office of the hospital on or before 4 PM on 12th June 2026


General Manager

